

## SulfaVer 4 Method<sup>1</sup>

**Method 10248**
**2 to 70, 20 to 700, 200 to 7000 mg/L SO<sub>4</sub><sup>2-</sup>**
**Powder Pillows**

**Scope and application:** For brine solutions, produced waters and hydraulic fracturing waters.

<sup>1</sup> Adapted from *Standard Methods for the Examination of Water and Wastewater*, SM4500-SO<sub>4</sub><sup>2-</sup>-E.




### Test preparation

## Instrument-specific information

Table 1 shows all of the instruments that have the program for this test. The table also shows sample cell and orientation requirements for reagent addition tests, such as powder pillow or bulk reagent tests.

To use the table, select an instrument, then read across to find the applicable information for this test.

**Table 1 Instrument-specific information**

Instrument	Sample cell orientation	Sample cell
DR6000 DR3800 DR2800 DR2700 DR1900	The fill line is to the right.	2495402 
DR5000 DR3900	The fill line is toward the user.	
DR900	The orientation mark is toward the user.	2401906 

## Before starting

For turbidimetric methods, install the instrument cap or cover on all instruments before ZERO or READ is pushed.

Use the Standard Adjust option with each new lot of reagent for the best results. Refer to the Standard solution method in [Accuracy check](#) on page 4.

For the best results, measure the reagent blank value for each new lot of reagent. Replace the sample with deionized water in the test procedure to determine the reagent blank value. Subtract the reagent blank value from the sample results automatically with the reagent blank adjust option.

Filter samples that are turbid with filter paper and a funnel.

Do not use the Pour-Thru Cell or sipper module (for applicable instruments) with this test.

The reagents that are used in this test contain barium chloride. Collect the reacted samples for safe disposal.

Review the Safety Data Sheets (MSDS/SDS) for the chemicals that are used. Use the recommended personal protective equipment.

Dispose of reacted solutions according to local, state and federal regulations. Refer to the Safety Data Sheets for disposal information for unused reagents. Refer to the environmental, health and safety staff for your facility and/or local regulatory agencies for further disposal information.

## Items to collect



Description	Quantity
SulfaVer® 4 Reagent Powder Pillows, 10-mL	1
Sample cells (For information about sample cells, adapters or light shields, refer to <a href="#">Instrument-specific information</a> on page 1.)	1

Refer to [Consumables and replacement items](#) on page 5 for order information.

## Sample collection and storage

- Collect samples in clean glass or plastic bottles.
- To preserve samples for later analysis, keep the samples at or below 6 °C (43 °F) for up to 28 days.
- Let the sample temperature increase to room temperature before analysis.

## Powder pillow procedure

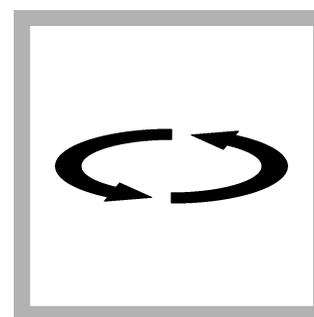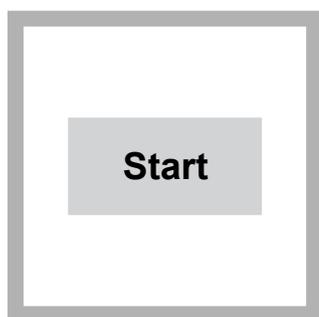

**1. Start program 680 Sulfate.** For information about sample cells, adapters or light shields, refer to [Instrument-specific information](#) on page 1.





**2. Add the sample volume** that is specified for the test range to a sample cell:

- 2–70 mg/L: 10 mL
- 20–700 mg/L: 1.0 mL
- 200–7,000 mg/L: 0.1 mL

Use a TenSette Pipet or glass pipet to measure 0.1 mL or 1.0 mL.

**3. If the sample volume is less than 10-mL add deionized water to the 10-mL line.** For the dilution factor, refer to [Set the dilution factor](#) on page 3.

**4. Swirl to mix.**

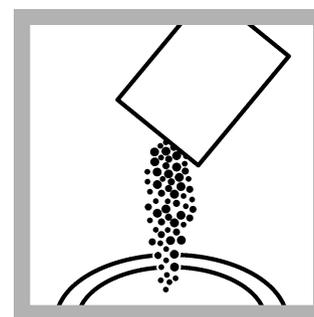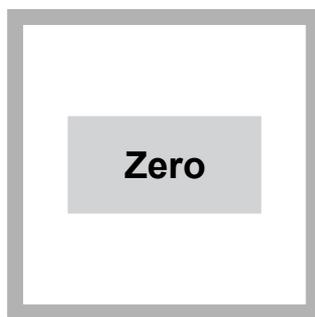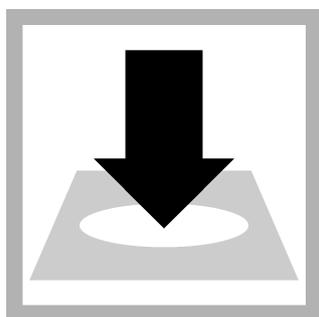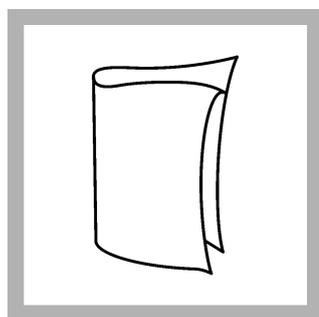


**5. Clean the blank sample cell.**

**6. Insert the blank into the cell holder.**

**7. Push ZERO.** The display shows 0 mg/L SO<sub>4</sub><sup>2-</sup>.


**8. Add the contents of one SulfaVer 4 Reagent Powder Pillow to the sample cell.** The sample will get cloudy if sulfate is present in the sample.

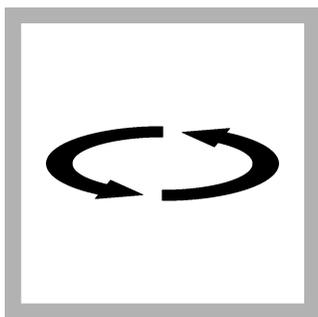


9. Swirl the sample cell to mix. Undissolved powder will not affect accuracy.




10. Start the instrument timer. A 5-minute reaction time starts.  
Do not move the sample cell during the reaction period.

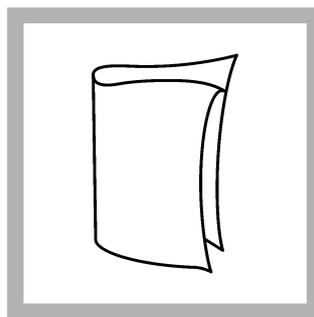


11. Clean the prepared sample cell.

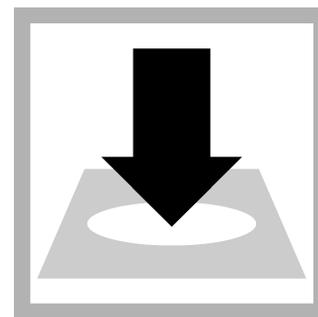

12. Within 5 minutes after the timer expires, insert the prepared sample into the cell holder.

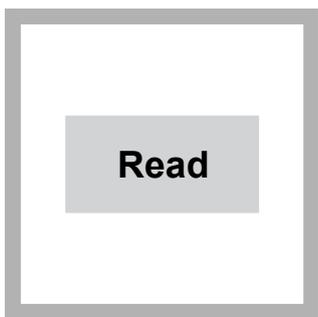

13. Push **READ**. Results show in mg/L  $\text{SO}_4^{2-}$ .

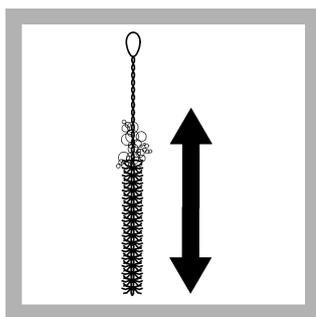

14. Clean the sample cell immediately after each test with soap, water and a brush.

## Interferences

Interfering substance	Interference level
Barium	Interferes at all levels. The higher the relative barium concentration when compared to the sulfate concentration, the higher the error. Samples with high barium concentrations will generally give a result that is 20% lower than the actual sulfate concentration.
Calcium	More than 20,000 mg/L as $\text{CaCO}_3$
Chloride	More than 40,000 mg/L as $\text{Cl}^-$
Magnesium	More than 10,000 mg/L as $\text{CaCO}_3$
Silica	More than 500 mg/L $\text{SiO}_2$

## Set the dilution factor

Instruments that have a dilution factor option can include the dilution factor in the result and show the concentration of the original, undiluted sample. For example, if the sample is diluted by a factor of 10, the instrument multiplies the result by 10 and shows the calculated result in the instrument display.

- Select **Options>More>Dilution** factor from the instrument menu.  
**Note:** DR1900: Select **Options>Advanced Options>Dilution Factors>On**.  
**Note:** Colorimeters include a dilution factor when the chemical form is set. Go to **Options>Advanced Options>Chemical Form** and select LR, MR or HR.
- Enter the dilution factor:
  - 1 mL sample diluted to 10 mL: dilution factor is 10.
  - 0.1 mL sample diluted to 10 mL: dilution factor is 100.

- 
3. Push **OK** to confirm. Push **OK** again.
  4. Push **RETURN** to go back to the measurement screen.

## Accuracy check

### Standard additions method (sample spike)

Use the standard additions method (for applicable instruments) to validate the test procedure, reagents and instrument and to find if there is an interference in the sample.

Items to collect:

- Sulfate Ampule Standard Solution, 2500 mg/L sulfate
  - Ampule breaker
  - Pipet, TenSette®, 0.1–1.0 mL and tips
  - Mixing cylinders (3x), 25 mL
1. Use the test procedure to measure the concentration of the sample, then keep the (unspiked) sample in the instrument.
  2. Go to the Standard Additions option in the instrument menu.
  3. Select the values for standard concentration, sample volume and spike volumes.
  4. Open the standard solution.
  5. Prepare three spiked samples: use the TenSette pipet to add 0.1 mL, 0.2 mL and 0.3 mL of the standard solution, respectively, to three 25-mL portions of fresh sample. Mix well.
  6. Use the test procedure to measure the concentration of each of the spiked samples. Start with the smallest sample spike. Measure each of the spiked samples in the instrument.
  7. Select **Graph** to compare the expected results to the actual results.

***Note:** If the actual results are significantly different from the expected results, make sure that the sample volumes and sample spikes are measured accurately. The sample volumes and sample spikes that are used should agree with the selections in the standard additions menu. If the results are not within acceptable limits, the sample may contain an interference.*

### Standard solution method

Use the standard solution method to validate the test procedure, the reagents and the instrument.

Items to collect:

- Sulfate standard solution, 1000 mg/L
  - 100-mL volumetric flask, Class A
  - 5-mL volumetric pipet, Class A and pipet filler safety bulb
  - Deionized water
1. Prepare a 50 mg/L sulfate standard solution as follows:
    - a. Use a pipet to add 5.0 mL of 1000 mg/L sulfate standard solution into the volumetric flask.
    - b. Dilute to the mark with deionized water. Mix well. Prepare this solution daily.
  2. Use the test procedure to measure the concentration of the prepared standard solution.
  3. Compare the expected result to the actual result.

***Note:** The factory calibration can be adjusted slightly with the standard adjust option so that the instrument shows the expected value of the standard solution. The adjusted calibration is then used for all test results. This adjustment can increase the test accuracy when there are small variations in the reagents or instruments.*

## Method performance

The method performance data that follows was derived from laboratory tests that were measured on a spectrophotometer during ideal test conditions. Users can get different results under different test conditions.

Program	Standard	Precision (95% confidence interval)	Sensitivity Concentration change per 0.010 Abs change
680	40 mg/L SO <sub>4</sub> <sup>2-</sup>	30–50 mg/L SO <sub>4</sub> <sup>2-</sup>	0.4 mg/L SO <sub>4</sub> <sup>2-</sup>

## Summary of method

Sulfate ions in the sample react with barium in the SulfaVer 4 and form a precipitate of barium sulfate. The amount of turbidity formed is proportional to the sulfate concentration. The measurement wavelength is 450 nm for spectrophotometers or 520 nm for colorimeters.

## Pollution prevention and waste management

Reacted samples contain barium and must be disposed of as a hazardous waste. Dispose of reacted solutions according to local, state and federal regulations.

## Consumables and replacement items

### Required reagents

Description	Quantity/test	Unit	Item no.
SulfaVer <sup>®</sup> 4 Reagent Powder Pillow <sup>1</sup> , 10-mL	1	100/pkg	2106769

### Recommended standards

Description	Unit	Item no.
Sulfate Standard Solution, 1000-mg/L as SO <sub>4</sub> <sup>2-</sup>	500 mL	2175749
Sulfate Standard Solution, 2500-mg/L, 10-mL ampules as SO <sub>4</sub> <sup>2-</sup>	16/pkg	1425210

### Optional reagents and apparatus

Description	Unit	Item no.
Mixing cylinder, graduated, 25 mL	each	189640
Mixing cylinder, graduated, 50 mL	each	189641
Ampule Breaker, 10-mL Voluette <sup>®</sup> Ampules	each	2196800
Pipet, volumetric 5.00-mL	each	1451537
Pipet filler	1	1465000
Pipet, TenSette <sup>®</sup> , 0.1–1.0 mL	each	1970001
Pipet tips for TenSette <sup>®</sup> Pipet, 0.1–1.0 mL	50/pkg	2185696
Pipet, TenSette <sup>®</sup> , 1.0–10.0 mL	each	1970010
Pipet tips for TenSette <sup>®</sup> Pipet, 1.0–10.0 mL	50/pkg	2199796
Flask, volumetric, Class A, 100 mL, glass	each	1457442

<sup>1</sup> SulfaVer is a registered trademark of Hach Company.



**FOR TECHNICAL ASSISTANCE, PRICE INFORMATION AND ORDERING:**  
In the U.S.A. – Call toll-free 800-227-4224  
Outside the U.S.A. – Contact the HACH office or distributor serving you.  
On the Worldwide Web – [www.hach.com](http://www.hach.com); E-mail – [techhelp@hach.com](mailto:techhelp@hach.com)

**HACH COMPANY**  
WORLD HEADQUARTERS  
Telephone: (970) 669-3050  
FAX: (970) 669-2932